

# Capio™ Slim


Suture Capturing Device



# Capio™ SLIM

## Suture Capturing Device

The Capio SLIM Suture Capturing device features a reduced profile to minimize the space required within the surgical field, easy suture loading and a funnel shaped catch, designed for consistent ease of use.

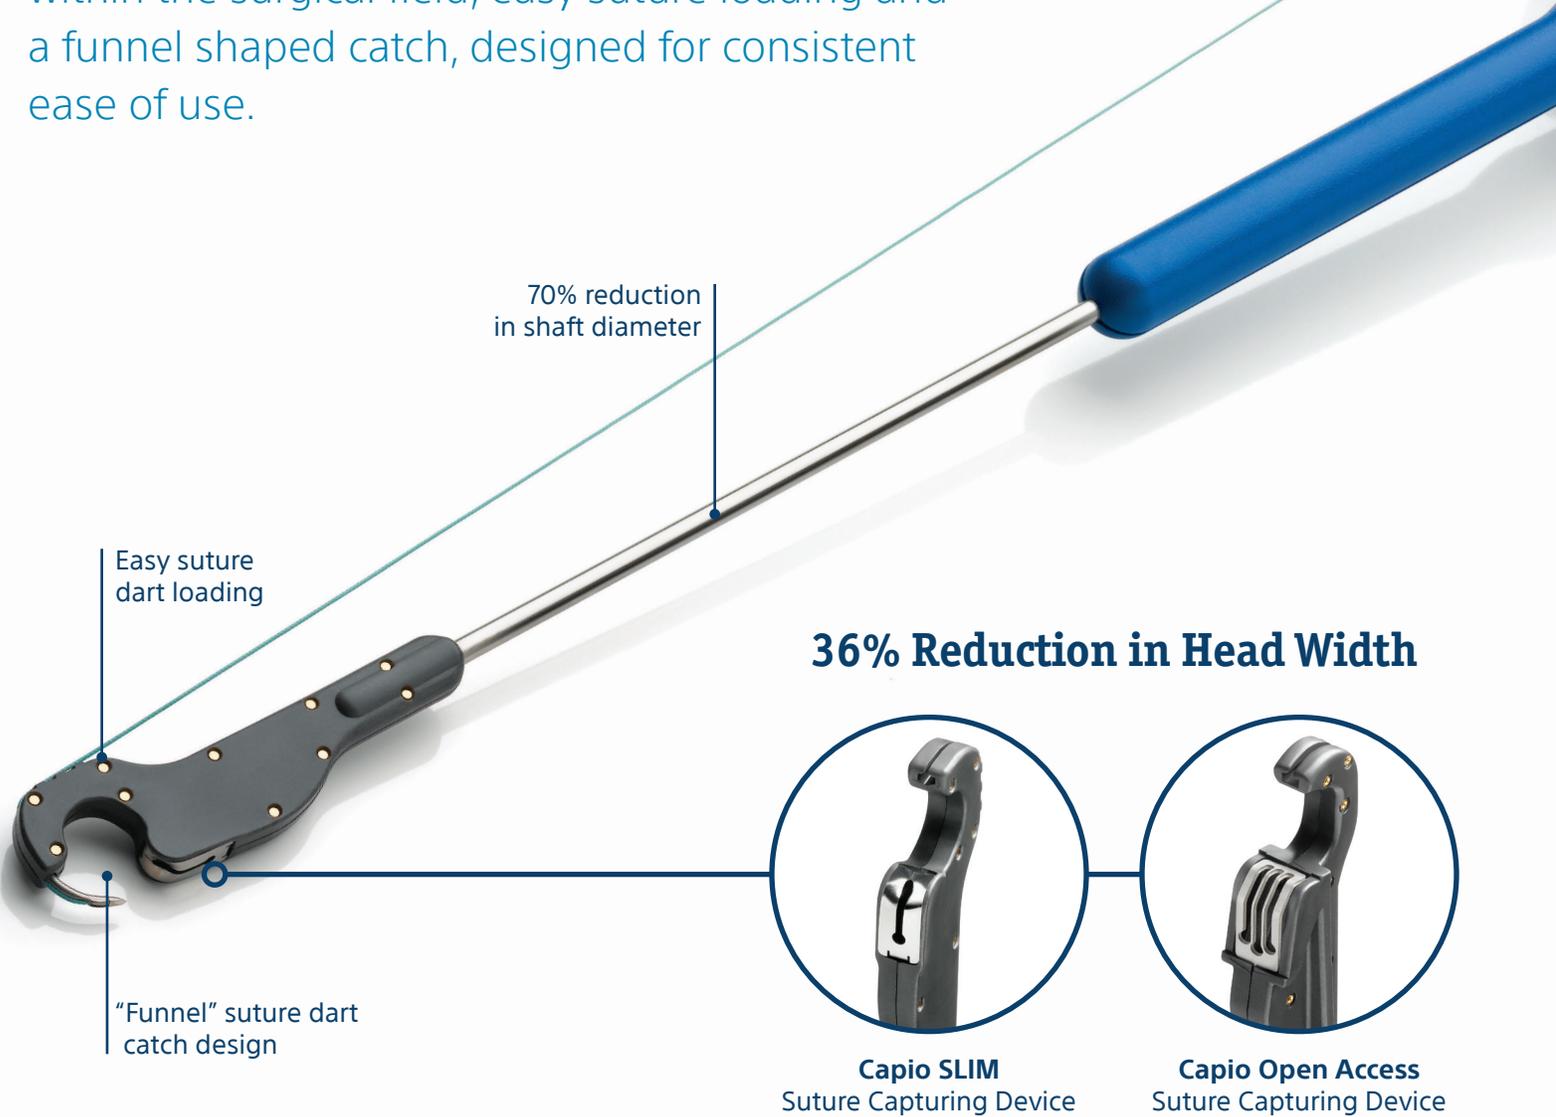

## The evolution continues with the Capio SLIM Suture Capturing Device

Since 1995, the Capio Device has provided consistent suture placement in difficult to access



**1995**

The Capio Suture Capturing Device debuts, revolutionizing the field of urogynecology.



**1999**

Capio Device may be used with other biological graft materials offering another treatment option



Ergonomic handle providing 3 finger grip

## Comparison of Suture Capturing Device Heads

Building on the history and reducing the profile, the Capio SLIM Suture Capturing Device features one of the smallest device profiles and suture dart carrier diameter while keeping the same bite depth as the current Capio Open Access Suturing Device.


**Capio™ SLIM**  
Suture Capturing Device



**Digitex™**  
Suture Delivery System



**FiXT™**  
Suturing Device



**Figure 1:** Comparison of Device Heads illustrates the difference in carrier diameter amongst these fixation devices. The Capio SLIM Suture Capturing Device carrier diameter is 45% less than the FiXT Suturing Device, 43% less than the Digitex Suture Delivery System.

## Fixation Device Comparison

	Shaft Diameter	Head Width	Device Weight	Carrier Diameter
<b>Capio OPEN ACCESS</b> Suture Capturing Device**	10.1 mm	9.8 mm	45.4 g	1.2 mm
<b>Capio SLIM</b> Suture Capturing Device*	3.0 mm	6.3 mm	38.2 g	1.2 mm
<b>Digitex Suture</b> Delivery System*	9.5 mm	9.6 mm	133.3 g	2.1 mm
<b>FiXT</b> Suturing Device*	4.8 mm	6.9 mm	121.1 g	2.2 mm

**Figure 2:** Fixation Device Comparison illustrates the device profile differences amongst these fixation devices. The Capio SLIM Suture Capturing Device has the smallest device profile based on the following measurements: shaft diameter, head width and device weight.

\* Measurements were recorded using one (1) of each device. Data on file at Boston Scientific.

\*\* Head width and device weight values are an average of five (5) device measurement recordings. Shaft diameter values are an average of fifteen (15) device measurement recordings. Data on file at Boston Scientific.

pelvic floor locations.



**2011**

The Capio Device remains "the foundation" of Pelvic Floor Reconstruction.



**2012**

Capio SLIM: the evolution continues.

# Capio™ Slim Suture Capturing Device

Order Number	Description	Unit
M0068318250	Capio Slim Suture Capturing Device	bx 1
M0068318261	Capio Slim Suture Capturing Device	bx 5

## Capio Sutures

Order Number	Description	Size	Unit
M0068332231	Non-absorbable, coated braided polyester, double armed with TC tapercut needle (dart), 48"	0	bx 12
M0068332341	Non-absorbable, polypropylene monofilament, double armed with TC tapercut needle (dart), 48"	0	bx 12
M0068332451	Absorbable, coated braided PGA, double armed with TC tapercut needle (dart), 48"	0	bx 12
M0068332241	Non-absorbable, coated braided polyester, double armed with TC tapercut needle (dart) and a T 26mm 1/2 circle taper needle, 36"	0	bx 12
M0068332351	Non-absorbable, polypropylene monofilament, double armed with TC tapercut needle (dart) and a T 26mm 1/2 circle taper needle, 36"	0	bx 12
M0068331371	Monodek™ Absorbable, monofilament PDO, double armed with TC tapercut needle (dart) and a T 26mm 1/2 circle taper needle, 48"	0	bx 12

## Your pelvic floor reconstructive tool to meet a variety of your algorithm needs:

- Native tissue repair
- Biologic graft augmentation
- And more...

**Boston  
Scientific**  
Advancing science for life™

Boston Scientific Corporation  
300 Boston Scientific Way  
Marlborough, MA 01752  
www.bostonscientific.com

**Ordering Information**  
**1.888.272.1001**

© 2021 Boston Scientific Corporation  
or its affiliates. All rights reserved.

WH-125306-AE MAY 2019

All images are owned by Boston Scientific. All trademarks are the property of their respective owners.

CAUTION: Federal Law (USA) restricts these devices to sale by or on the order of a physician. Refer to package insert provided with these products for complete Indications for Use, Contraindications, Warnings, Precautions, Adverse Events, and Instructions prior to using these products.

All trademarks are the property of their respective owners.